

Non-Contact Thermometer

User's Manual

THERMO-HUNTER® BUILT-IN2

BA-30TC BA-06TC

Thank you for purchasing Optex products.

- Please check to make sure the model you purchased in the model you specified.
- Please read the manual before using the "Thermohunter Built-in 2" in order to use it correctly.
- After reading the manual, please be sure to keep it for future reference.



OPTEX CO.,LTD.

5-8-12 Ogoto Otsu Shiga 520-0101 Japan
TEL.+81-77-579-8680 FAX.+81-77-579-8199

"Take Care of Environment." This manual uses recycled paper.

PRINTED IN JAPAN 1034-4 2008/2

Safe Usage


This user's manual contains various warnings to ensure safe usage of the product and prevent damage and injury to you and other persons. Please be sure to heed the warnings and strictly follow safety procedures.



This symbol signifies that improper usage may result in injuries or damage.


- ⊘ : This symbol signifies a prohibited action.
- ⓘ : This symbol signifies a required action.

CAUTION



Please don't look at the laser directly or aim it toward the eyes. The laser may cause eye injury or damage to your health.

CAUTION



This product is not a clinical thermometer and therefore, cannot be used medical purposes.

Environmental Warnings

KEEP THE THERMOMETER AWAY FROM DIRECT SUNLIGHT, DUST, HIGH TEMPERATURES AND HIGH HUMIDITY DURING USE AND STORAGE.
Otherwise, the optical lens will become dirty or damaged. Such usage or storage will result in incorrect measurements.

DO NOT APPLY SUDDEN CHANGE OF ENVIRONMENTAL TEMPERATURE TO THE THERMOMETER.

Sudden temperature changes of environments may cause incorrect measuring results. In such cases, leave the thermometer for a moment to let it return to a stable condition prior to the next measurement.

KEEP THE THERMOMETER AWAY FROM PRODUCTS WHICH PRODUCE STRONG ELECTROMAGNETIC WAVES. DO NOT USE IN AN ATMOSPHERE CONTAINING CORROSIVE GASES OR EXPLOSIVE GASES.

Usage in such environments will cause irreparable damages to the unit and incorrect measurements.

Usage Warnings

AVOID MEASURING SHINY OBJECTS.
Shiny objects reflect surrounding temperatures. The emissivity rate of the unit can be adjusted to compensate for this problem.


DO NOT USE WITH NON-STANDARD VOLTAGE.
Using the unit out of DC 12~24 voltage range may result in damage to the unit, shorts, fires and injuries. In such cases, immediately switch the unit off.

DO NOT TOUCH TO THE OBJECTS THAT IS BEING MEASURED.
The unit is a non-contact thermometer. Touching the unit to objects with high temperatures will result in irreparable damages in the shape of the unit and incorrect measurements.

DO NOT TOUCH THE LENS.
Do not touch the lens with hard or sharp objects. Do not insert foreign objects into the light receiving part. Otherwise, damage to the lens or incorrect measurements will occur.


DO NOT USE NEAR ELECTRIFIED OBJECTS.
Otherwise, irreparable damages or incorrect measurements will result.

Name and Usage of Each Product Part

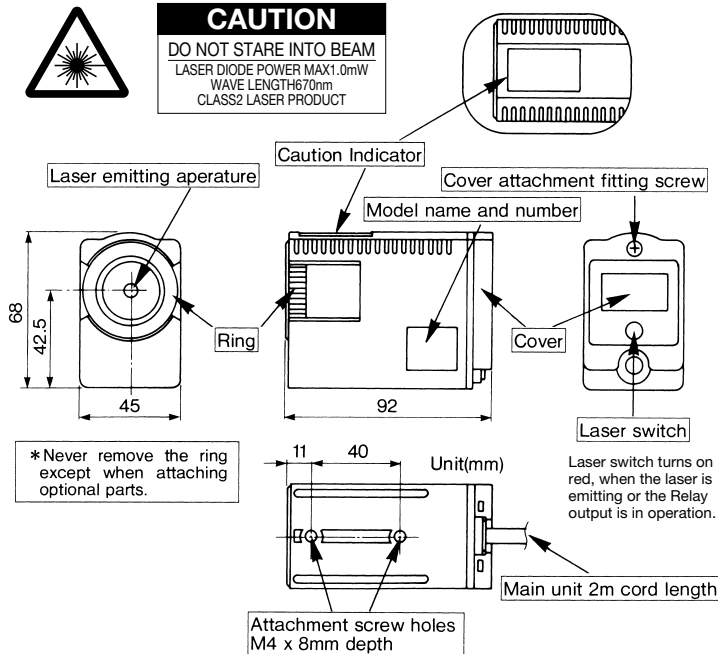

1. Installation

1. Please firmly install using the attachment screw holes on the lower section of the main unit while strictly following the warnings below. Please use the M4 screws provided. When using screws sold on the market, please do not use attachment screws over 8mm in length.

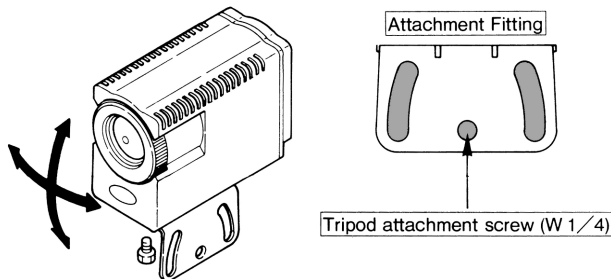


○ It is possible to angle the product by 45 degrees upward/downward or left/right if the provided attachment fittings are used. The two taps of the attachment fittings are the tripod attachment screws (W1/4). By screwing the attachment fittings onto the main unit, the product can be attached to the tripod.

Installation Warnings

1. Please install the unit so that the product is perpendicular to the object to be measured.
2. Please install the unit so that the cover can be attached and removed.
3. Please install the unit so that the main unit doesn't vibrate or receive shocks.
4. Please check to make sure that there are no sources of heat near the main unit or object to be measured. Highly reflective objects may cause discrepancies in measurement.
5. Please install the unit in a location which isn't subject to direct hot air and where surrounding temperatures do not exceed 50°C.

2. Connection

1. Please make the connections correctly as shown in the illustration below while strictly following the warnings.

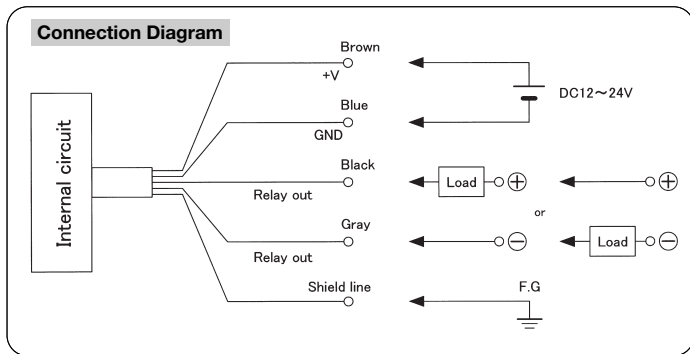

Connection Warnings


1. Use the unit within rated voltage and confirm proper wiring sufficiently for the connection.
2. Do not short-circuit Relay output with another output cable.
3. As photo MOS relay is used for the relay output, it is isolated from a circuit. On-resistor is 2.5Ω or less.
4. In case of using the unit in the strong EMI noise environment, it is necessary to run the output cable through an iron pipe, etc., as a precaution.

3. Measurement

1. Turn the unit on after checking to see there are no mistakes in connection. The LCD display will light up.
2. Press the laser switch, and the laser marker will light up. Check to see that the laser is aimed at the center area of the object to be measured. The laser marker is aimed at the center of the area to be measured. Press the laser switch again to turn it off or wait 20 seconds, and it will automatically turn off.
3. Follow each step in "4. Setting."
4. Check to see if the unit is operating normally.

4. Setting

1. Take off the cover.
2. Press the Δ/∇ button to move the menu bar, and set it to the position you want. At this time, the flashing numerical figure will show the current setting figure.

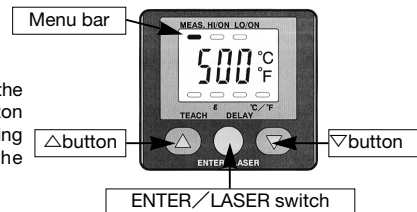


MEAS.	: Conduct a conventional measurement
TEACH	: Set the temperature (real temperature) of the object to be measured. Calculate the emissivity ratio from the real temperature. Automatically adjust the set figure of the emissivity ratio.
ε	: Set the emissivity ratio of the object to be measured. ε = 1.20~0.10 Adjust the measurement value according to the set emissivity ratio.
DELAY	: Select the response time. Set figure 1~200 (0.5~10 seconds) Smoothing is possible if setting when the display fluctuates or when you wish to see (produce) the average figure.
*C/°F	: Switch between temperature displays.
HI/ON	: Setting Relay output. When the measuring value rises above the preset value, Relay output is on.
LO/ON	: Setting Relay output. When the measuring value is lower than the preset value, Relay output is on.

3. Press the ENTER button to put into "SET MODE". For the TEACH and emissivity setting, the laser marker lights up.
4. Press the Δ/∇ button to change the set figure. At this time, the figure which is displayed alternately with the set figure represents the operand temperature of the set figure/value.
5. Press the ENTER button to record. At this time, the blinking numerical figure, etc., represents the set figure after change.
6. Press the Δ/∇ button to return the menu bar to the MEAS. position and put into "MEASURE MODE." The unit will automatically return to "MEASURE MODE" if no buttons are pushed for a period greater than 10 seconds. At this time, setting is invalid.

Relay output setting

1. Move the menu bar to HI/ON or LO/ON, press the ENTER button.
 2. Press the Δ/∇ button to change the pre-set value for Relay output and press the ENTER button to fix the value.
 3. Press the Δ/∇ button to set ON (effective) or OFF (ineffective), and press the ENTER button. In case of ON, the Relay output is effective, after the ENTER button is pressed.
- ※ When Relay output is effective, Enter button turns on. If the preset value of HI is set lower than of LO, the Relay output is effective when the Thermometer shows the measuring value within the range preset value between LO and HI.



TEACH Function

This is the function in case that the emissivity ratio of objects is unknown. Firstly, measure the temperature value of the target with Thermocouple, etc., then enter the result (temperature value measured) into Teach Mode. After the process, the emissivity ratio is automatically calculated and the Thermometer shows each measuring value according to the ratio. Teach-in function is not available while the display blinks or shows ERR. Use direct input of ε -value.

Emissivity ratio (ε)

The emissivity ratio is the rate of the energy emitted from the surface of the object. All objects possess a particular emissivity ratio which changes according to the object's surface conditions or temperature. Since the unit allows the emissivity ratio to be set, even more precise measurements can be conducted by matching the emissivity ratio of the object to be measured. Objects with a low emissivity ratio (e.g. the surface of shiny metallic objects) reflect the surrounding temperature since they are highly reflective. In this case, it is necessary to block out these effects from surrounding objects since incorrect measurements will result by reflecting these temperatures. The emissivity ratio normally has a maximum value of 1.00. However, taking into consideration the influence of surrounding noise, the unit can be set up to 1.20.

Maintenance

Lens

Dust, dirt and scratches on the lens cause incorrect measurements. In case of dirty lenses, please remove the dust on the lens with a blower, etc. for lens cleaning use. If the dust or dirt can not be removed with a blower, lightly wipe the lens with a cotton swab or special lens cleaning cloth using a little ethanol alcohol.

Main Unit

The main unit is made of PBT and polycarbonate. When it becomes dirty, lightly wipe caustic soda, ammonia, acetone, thinner, etc. to clean the dirt off since these chemicals will permeate the surface and melt it.

Calibration

We recommend a regular calibration. Please inquire at your distributor where you bought the unit.


Trouble shooting

Problems	Cause	Solution
Display doesn't appear	The power source is not connected properly. The power voltage is low.	Check the lead wires and the connections. Check the power voltage and adjust it to the DC12~24V range.
Laser doesn't appear, it is dark.	The laser emitting aperture is dirty.	Clean the lens referring to the Lens section under "Maintenance".
The measured figure is odd.	The lens is dirty. The measuring area is off center. Near the object to be measured is another object emitting high temperatures, affecting the temperature reading.	Clean the lens referring to the Lens section under "Maintenance". Adjust the laser marker so that it is aimed at the center of the object to be measured. Block the heat source using a board, etc.
The measured figure is not stable.	The emissivity ratio setting is off. The unit is vibrating. The temperature of the unit changes suddenly.	Reset to the emissivity ratio of the object to be measured. Prevent the vibration. Put the unit aside for a while to stabilize the unit's temperature.
Impossible to teach in. (ERR)	Unproper setting	Confirm again the setting value, or input ε value directly.


If the above solutions do not correct the problems or should other problems not mentioned above occur, please contact your distributor.

Field of View

BA-30TC

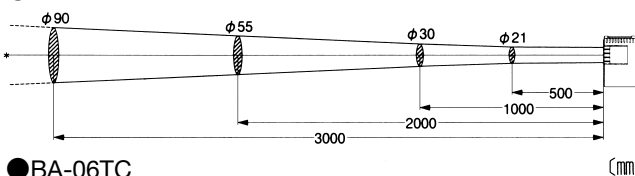

BA-06TC

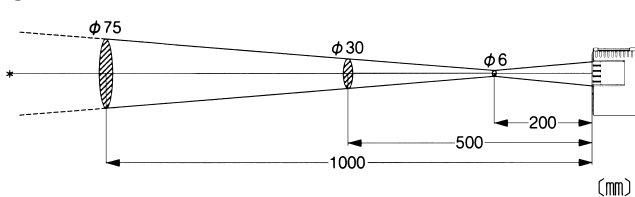

- * The laser marker is aimed at the center of the measuring area.
- * The optical resolution values stated in "Field of View" are at 90% energy.
- * The size of measuring object should be sufficiently larger than the "Field of View" (spot size) shown in the above illustration.

Specifications

Model	BA-06TC	BA-30TC
Temperature Range	0~500°C (display -20~520°C)	
Area Size	φ 6 / 200mm	φ 30 / 1000mm
Optics	Silicon lens	
Spectral Response	Thermopile / 8~14 μm	
Response Speed	500ms / 90%	
Accuracy	±1% of reading value or ±2°C ±1digit, whichever is greater (ε ≈ 1.0)	
Repeatability	±1°C of reading value	
Display Resolution	1°C	
Relay output	Photo Mos relay output, 350mA • DC100V Max	
Output Renewal Time	50ms	
Focus	Coaxial laser marker	
Emissivity ratio (ε) Adjustment	0.10~1.20	
Delay Function	Nominal 1~200 (0.5~10sec) variable	
Power Supply	DC12~24V ± 10% / MAX150mA	
Ambient temperature	0~50°C	
Environmental Humidity	35~85%RH (without dew condensation)	
Storage Temperature	-10~60°C	
Vibration Resistance	3G (20~50Hz, according to JIS CO911)	
Water Resistance	IP65	
Materials	Ring case : glass-containing PBT, Rear : PSF Cover : PC	
Weight	360g	

Accessories : Attachment Fitting ×1, M4 screw ×2

Optional accessories : Air purge collar : BA-AP1

* Design and specifications are subject to change for product improvement without prior notice.